

date 08/05/2022

page 1 of 3

# MODEL: HSS07-C20-P274 | DESCRIPTION: HEAT SINK

#### **FEATURES**

- TO-220 package
- solder pin
- copper alloy
- tin plated






#### thermal resistance1 power **MODEL** dissipation<sup>1</sup> @ 75°C ∆T, nat @ 1 W, @ 1 W, @ 1 W, @ 75°C ∆T, nat 400 LFM conv (°C/W) nat conv 200 LFM conv (°C/W) $(^{\circ}C/W)$ (°C/W) (W) HSS07-C20-P274 29.57 35.5 12.6 8.9 2.54

1. See performance curves for full thermal resistance details.

## PERFORMANCE CURVES

	Heatsink Temperature Rise Above Ambient (ΔT = Ths - Ta) (°C)		
Power (W)	Natural Conv.	200 LFM	400 LFM
0	0	0	0
1	35.5	12.6	8.9
2	64.5	24.6	17.7
3	90.9	36.6	26.3
4	115.1	49.3	35.2
5	137.4	60.4	43.8

Ths: "hot spot" temperature measured on the heatsink Ta: ambient temperature

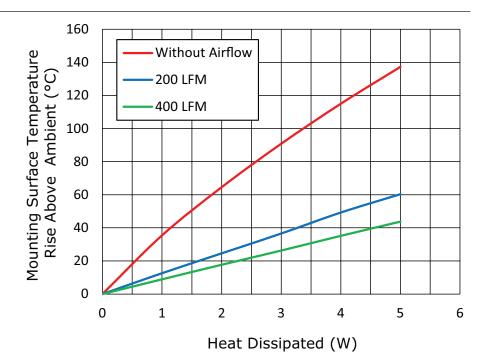



# **MECHANICAL DRAWING**


units: mm

tolerance: ±0.25 mm

MATERIAL	C1100
FINISH	tin
THICKNESS	0.6 mm
WEIGHT	4.5 g

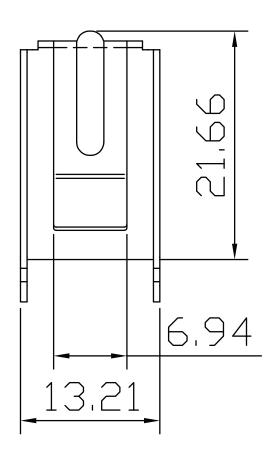

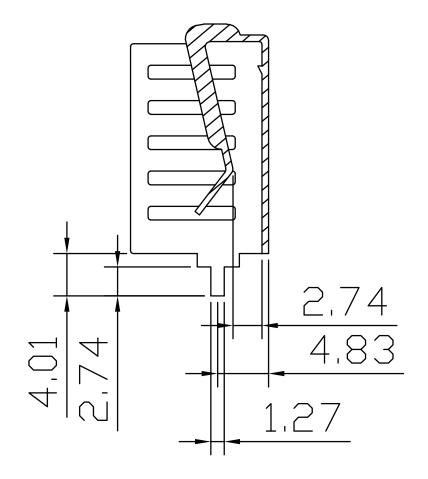



Additional Resources: Product Page | 3D Model

CUI DEVICES | MODEL: HSS07-C20-P274 | DESCRIPTION: HEAT SINK

**date** 08/05/2022 | **page** 3 of 3

### **REVISION HISTORY**

rev.	description	date
1.0	initial release	06/25/2021
1.01	logo, datasheet style update	08/05/2022

The revision history provided is for informational purposes only and is believed to be accurate.



CUI Devices offers a one (1) year limited warranty. Complete warranty information is listed on our website.

CUI Devices reserves the right to make changes to the product at any time without notice. Information provided by CUI Devices is believed to be accurate and reliable. However, no responsibility is assumed by CUI Devices for its use, nor for any infringements of patents or other rights of third parties which may result from its use.

CUI Devices products are not authorized or warranted for use as critical components in equipment that requires an extremely high level of reliability. A critical component is any component of a life support device or system whose failure to perform can be reasonably expected to cause the failure of the life support device or system, or to affect its safety or effectiveness.