

date 08/05/2022

page 1 of 4

# MODEL: CUSA-TR09-02-1000-TH67 | DESCRIPTION: ULTRASONIC SENSOR

#### **FEATURES**

- · aluminum can
- IP67 rated
- · combination unit: receiver & transmitter
- high frequency









parameter	conditions/description	min	typ	max	units
type	transmitter/receiver				
operating voltage	at 200 kHz			500	Vp-p
frequency		185	200	215	kHz
echo sensitivity	at 0.2 m	1,800			mV
directivity	at -6 dB	7	9	11	degree
capacitance	at 1 kHz	420	600	780	pF
detectable range		D.1		2.0	m
response time	at 200 Vp-p, 200 kHz			0.58	ms
dimensions	Ø19 x 11				mm
material	aluminum				
terminal	pins (brass with tin plating)				
weight			6.4		g
operating temperature		-40		80	°C
storage temperature		-40		85	°C
RoHS	yes				
IP level	IP67				


# **SOLDERABILITY**

parameter	conditions/description	min	typ	max	units
wave soldering				260	°C

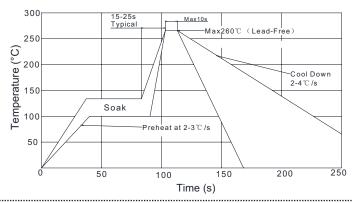


# **MECHANICAL DRAWING**

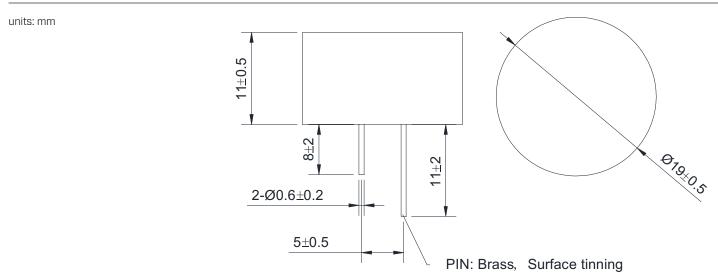

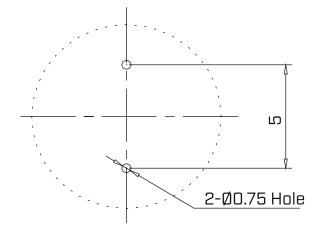

Recommended PCB Layout Top View


### **BEAM PATTERNS**

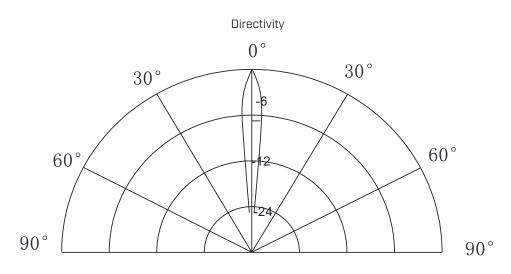

# **PACKAGING**

units: mm

Tray Size: 235 x 135 x 30 mm Tray QTY: 50 pcs per tray Carton Size: 280 x 285 x 240 mm Carton QTY: 1,000 pcs per carton

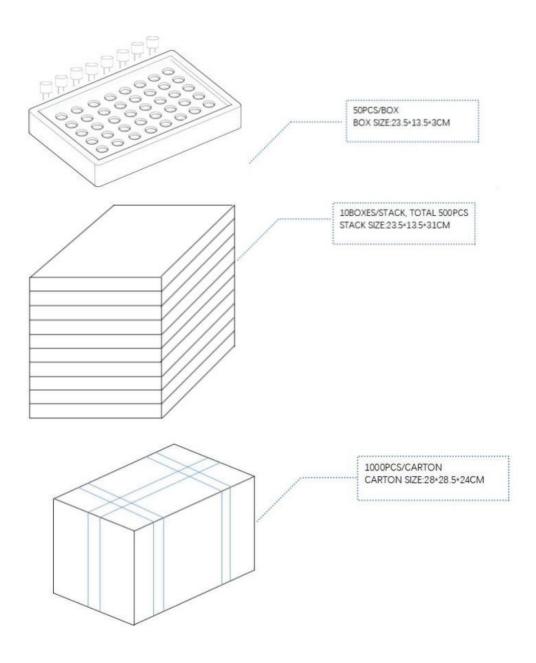

#### **REVISION HISTORY**

rev.	description	date	
1.0	initial release	05/24/2022	
1.01	logo, datasheet style update	08/05/2022	

The revision history provided is for informational purposes only and is believed to be accurate.



CUI Devices offers a one (1) year limited warranty. Complete warranty information is listed on our website.

CUI Devices reserves the right to make changes to the product at any time without notice. Information provided by CUI Devices is believed to be accurate and reliable. However, no responsibility is assumed by CUI Devices for its use, nor for any infringements of patents or other rights of third parties which may result from its use.

CUI Devices products are not authorized or warranted for use as critical components in equipment that requires an extremely high level of reliability. A critical component is any component of a life support device or system whose failure to perform can be reasonably expected to cause the failure of the life support device or system, or to affect its safety or effectiveness.